

Currently Adopted Criteria for Pedicle Screw Diameter Selection

Giovanni F. Solitro, Keith Whitlock, Farid Amirouche, Ankit I. Mehta and Annie McDonnell

Int J Spine Surg published online 12 April 2019
<https://www.ijssurgery.com/content/early/2019/04/12/6018>

This information is current as of February 20, 2025.

Email Alerts Receive free email-alerts when new articles cite this article. Sign up at:
<http://ijssurgery.com/alerts>

Currently Adopted Criteria for Pedicle Screw Diameter Selection

GIOVANNI F. SOLITRO,¹ KEITH WHITLOCK,² FARID AMIROUCHE,³ ANKIT I. MEHTA,⁴ ANNIE MCDONNELL⁵

¹Department of Orthopaedics, Louisiana State University Health Science Center, Shreveport, Louisiana, ²College of Medicine, University of Illinois at Chicago, Chicago, Illinois, ³Department of Orthopaedics, University of Illinois at Chicago, Chicago, Illinois, ⁴Department of Neurosurgery, University of Illinois at Chicago, Chicago, Illinois, ⁵Department of Mechanical Engineering, University of Illinois at Chicago, Chicago, Illinois

ABSTRACT

Background: Transpedicular screw insertion has become widely accepted for the correction of spinal deformity as well as degenerative and traumatic injury, but adoption of this technique has remained less widespread in the thoracic compared to the lumbar spine. This is thought to be associated with the relative technical difficulty of screw insertion into the narrower widths of the thoracic pedicles and the neurologic and mechanical risks associated with breach of the pedicle wall. The surgical decision making involves determining the appropriate sized screw for maximum fixation strength while simultaneously respecting the structural integrity of the vertebral pedicles to prevent a breach and provide better fixation. This paper presents a systematic review of criteria for thoracic pedicle screw diameter (SD) selection in order to orient inexperienced surgeons on the impact of this selection on pedicle breaching and fixation strength.

Methods: We performed a systematic literature review focused on studies reporting SD selection in relation to pedicle dimensions, measures of fixation strength, and breach rate.

Results: Twenty-nine articles that measured fixation strength, breach rate, and/or provided SD in relation to pedicle width were selected for inclusion.

Conclusions: A commonly accepted criteria for pedicle SD selection has not yet been proposed. Screw diameters approximately 80% of the pedicle width have been adopted, but this proportion is rarely reported in the midthoracic vertebrae for which smaller pedicles and inadequate hardware specificity result in higher breach rates. Depending upon the insertion technique adopted, greater specificity in diameter selection by vertebral level should be pursued in order to maximally target cortical bone purchase.

Clinical Relevance: Based on this review of the literature, we believe that proper selection of the SD for individual vertebral level directly affects the insertion technique and the potential breach.

Other & Special Categories

Keywords: pedicle screws, bone fixation, fusion, thoracic spine, spine instrumentation

INTRODUCTION

Transpedicular screw insertion has become the gold standard for spinal fixation used in the correction of spinal deformity^{1–3} and trauma.^{4–7} It is focused on achieving long-lasting fixation and strength and providing the scaffolding for a bony fusion. Despite the increased use of pedicle screw constructs, the insertion of pedicle screws in the thoracic spine represents unique challenges as compared to the earlier adopted instrumentation of lumbar segments. These challenges mainly stem from the increased technical difficulty in placing thoracic pedicle screws due to smaller sized pedicles and the proximity to neural, visceral, and vascular structures of the thorax.^{8,9} Screw misplacement (see Figure 1) can alter the pullout strength (POS)¹⁰ and

can cause various complications such as intraoperative pedicle fracture, loosening, dural laceration, and transient neurologic injury.¹¹ The accuracy of screw insertion has been analyzed extensively, and full containment within the cortical walls of the pedicle is achieved 69–94% of the time using the free-hand technique, with an increased range of 89–100% of attempts when utilizing computer tomography (CT) navigation across all vertebral levels.¹² Additionally, a 2007 meta-analysis reporting on 130 studies representing 37 337 total screws reports an overall accuracy rate of 91.3% throughout the spine, with decreased accuracy at thoracic levels.¹³

It has been shown that, when using currently accepted insertional techniques, malposition is strongly reduced with surgeon experience.¹⁴ Chen

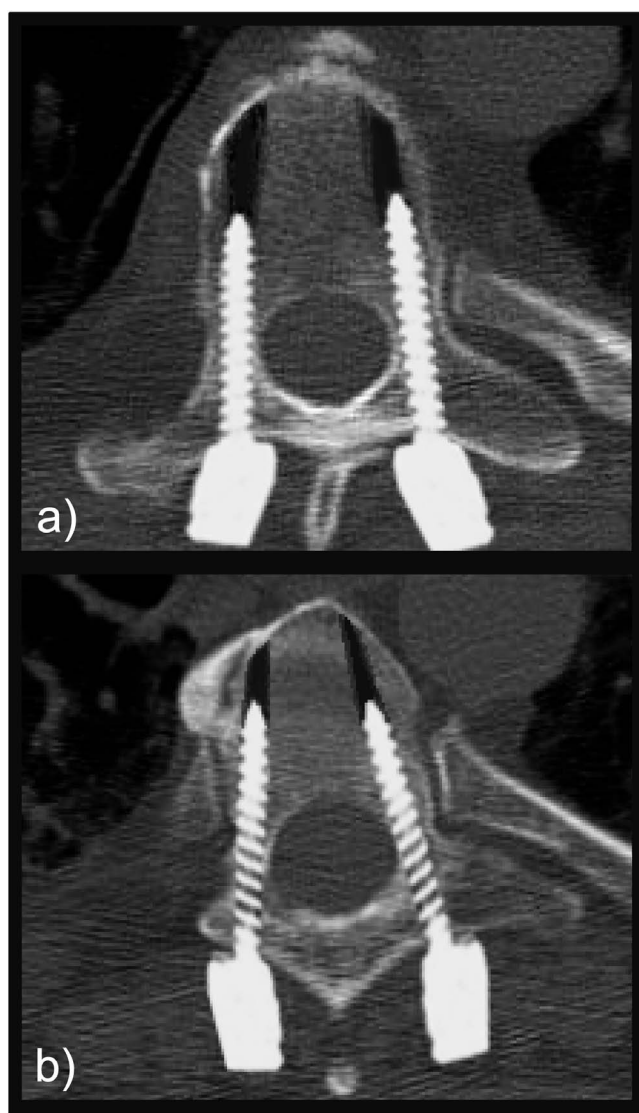


Figure 1. Pedicle screw insertion on computer generated images of (a) successfully placed screws and (b) misplaced screws: laterally for the right pedicle and medially for the left pedicle.

et al¹⁵ demonstrated that, using free-hand placement, an apprentice surgeon dangerously misplaced screws at a rate of 26.7%, in contrast to just 9.1% obtained by the chief surgeon. Furthermore, a minimum of 60 supervised screw placements were found to be necessary before the apprentice could accurately execute the free-hand technique independently. Additionally, in a 14-month period, Samdani et al¹⁶ reported a dangerous misplacement rate of 15.5% for a surgeon's first 181 implanted screws, which was reduced to 10.6% for the next 189 and 8.7% for the final 183 attempts. The selection of appropriate screw dimensions by vertebral level is key for successful insertion. As such, screw length is precisely pre-operatively and intraoperatively eval-

uated,^{17,18} but SD selection is left up to the experience of the surgeon.¹⁹ The tolerance for avoiding pedicle wall perforation has been theoretically proven to be reduced with increased SDs,²⁰ while in actual placement, the screw is selected as the largest possible^{17,19} to achieve greater stability.^{21,22} These measures are reported, often in separate studies, as experiments measuring either pullout/fixation strength or breach rate of screws inserted in vitro or in cadaveric models. The resultant compromise between safety and stability that must be weighed for SD selection remains an important area of research which the current study will review.

This study aims to build a comprehensive systematic review of thoracic pedicle SD selection in order to summarize currently suggested selection criteria and demonstrate the impact that this decision can have on pedicle breaching and fixation strength. We hope these findings will be of particular interest to inexperienced surgeons for whom the breach rate in relation to SD has been shown to be significantly higher.

MATERIALS AND METHODS

Search Strategy

A systematic literature search was conducted in PubMed, Scopus, EMBASE and Biomed Central online databases using the syntax: (((thoracic) AND pedicle) AND screw) AND diameter. Of the 423 articles identified by this strategy, duplicates were removed, yielding 290 articles eligible for review. Following this initial search, we conducted 2 additional searches with the keywords "size" and "width" in place of "diameter." After review, if articles were deemed worthy of inclusion, they were then checked against prior inclusions across all previous searches, and repeats were discarded. An additional 4 articles were also identified by hand search of the reference sections of articles identified by the review process.

Article Selection

Articles were selected for inclusion based on their contribution to 1 or more of 3 topics which we deemed relevant to our objective. These topics included (1) recommendations for appropriate SD selection including concurrent reporting of utilized SD and transverse pedicle dimension by vertebral level, (2) quantitative data on POS or insertional

torque of pedicle screws of defined diameter, and (3) quantitative data on breach rate of inserted pedicle screws of defined diameter. Studies meeting inclusion criteria (2–3) are all linked by the reporting of SD across defined vertebral level(s), allowing for useful comparison between groups. Studies were excluded during the review process for meeting 1 or more of our 8 exclusion criteria: (1) full text article was unavailable, (2) article was not available in English, (3) morphometric study without actual screw placement or description of ideal screw dimension, (4) article contained no significant/sufficient discussion of 1 or more keywords, (5) article consisted of analysis irrelevant to the topic, (6) article discussed cervical or lumbar spinal segments rather than thoracic, (7) article detailed a nonhuman study, and/or (8) studies related to bicortical screw placements. Extraction of relevant data by 2 independent observers followed the review process, and any discrepancies were resolved by the lead author. Given the heterogeneity of the studies involved in this systematic review, we determined early on that it would not be feasible to combine data across studies for use in a quantitative meta-analysis. Instead, we set out to individually examine each study in order to extract the relevant information about the relationships between diameter, strength, and safety, while considering the unique strengths and limitations of each study.

Screw Diameter Selection in Relation to Pedicle Widths

In an attempt to uniform the reported diameters to the documented pedicle dimensions, since pedicles are mostly evaluated in CT axial slices through their transverse width, we calculated the ratios of SD to pedicle width (PW) in studies where both values were reported. In order to compute these ratios, the standard deviations were dropped from the reported values and are thus to be considered as approximations. Average ratios were computed with standard deviations, representing the average ratio of SD to PW by vertebral level across studies. Additionally, we calculated the average breach rate by level as documented in literature, and using 3 of the most referenced morphological studies on the pedicle dimensions, we correlated the breach rate to the PWs and to the adopted SD/PW ratio performing linear regression in Microsoft Excel software (Microsoft Corp., Redmond, Washington).

RESULTS

Search Results

We identified 29 unique articles for inclusion in this review (see Figure 2). Among these studies, 18 provided information for SD selection in relationship to pedicle dimension, 10 reported quantifiable measures of fixation strength, and 10 reported values of breach rate. Studies providing recommendations for screw selection were often morphologic in nature and did not report data on safety/fixation strength of screw insertion. Of these, we reported the provided recommendations, and where possible, we calculated the SD to PW ratio, a measure that has been calculated in prior studies.^{23,24} Articles reporting fixation strength were further divided between those reporting POS of inserted screws and those reporting maximal insertional torque. Carmouche et al²¹ provided data on both of these measures of fixational strength and is thus listed twice in the summarizing table. There were 5 articles reporting measures of strength as well as PW^{22,25–28} and 4 articles reporting breach rate as well as PW.^{29–32}

Disclosed Criteria for Screw Diameter Selection

Articles which provided explicit recommendations for SD in relation to pedicle dimensions were highly variable (Table 1) and either consisted of a defined SD to PW ratio, a “pedicle fill” model,³³ or discussed the clearance necessary between the diameters of the screw and pedicle.

Suggested diameter values ranged from 80%²³ to no more than 125% of PW.²⁴ Two morphometric analyses of PW in different patient populations state that a 0.5 mm margin of cortical bone should be left on both the lateral and medial margins of the screw for safe fixation with both straightforward and anatomical insertion techniques.^{16,34}

An additional study by Christodoulou et al³⁵, in which the insertion technique is not indicated, simply suggests that SD should be matched as closely as possible to the internal cortical diameter of the pedicle without ever exceeding the outer cortical width. Furthermore, when these studies are grouped by the age of their relevant patient population, only those dealing at least in part with a pediatric population offered recommendations for SD wider than the pedicle.^{24,36,37} These studies, based on both insertion techniques, define the upper limits for pediatric SD/PW between 1.15 and 1.25.

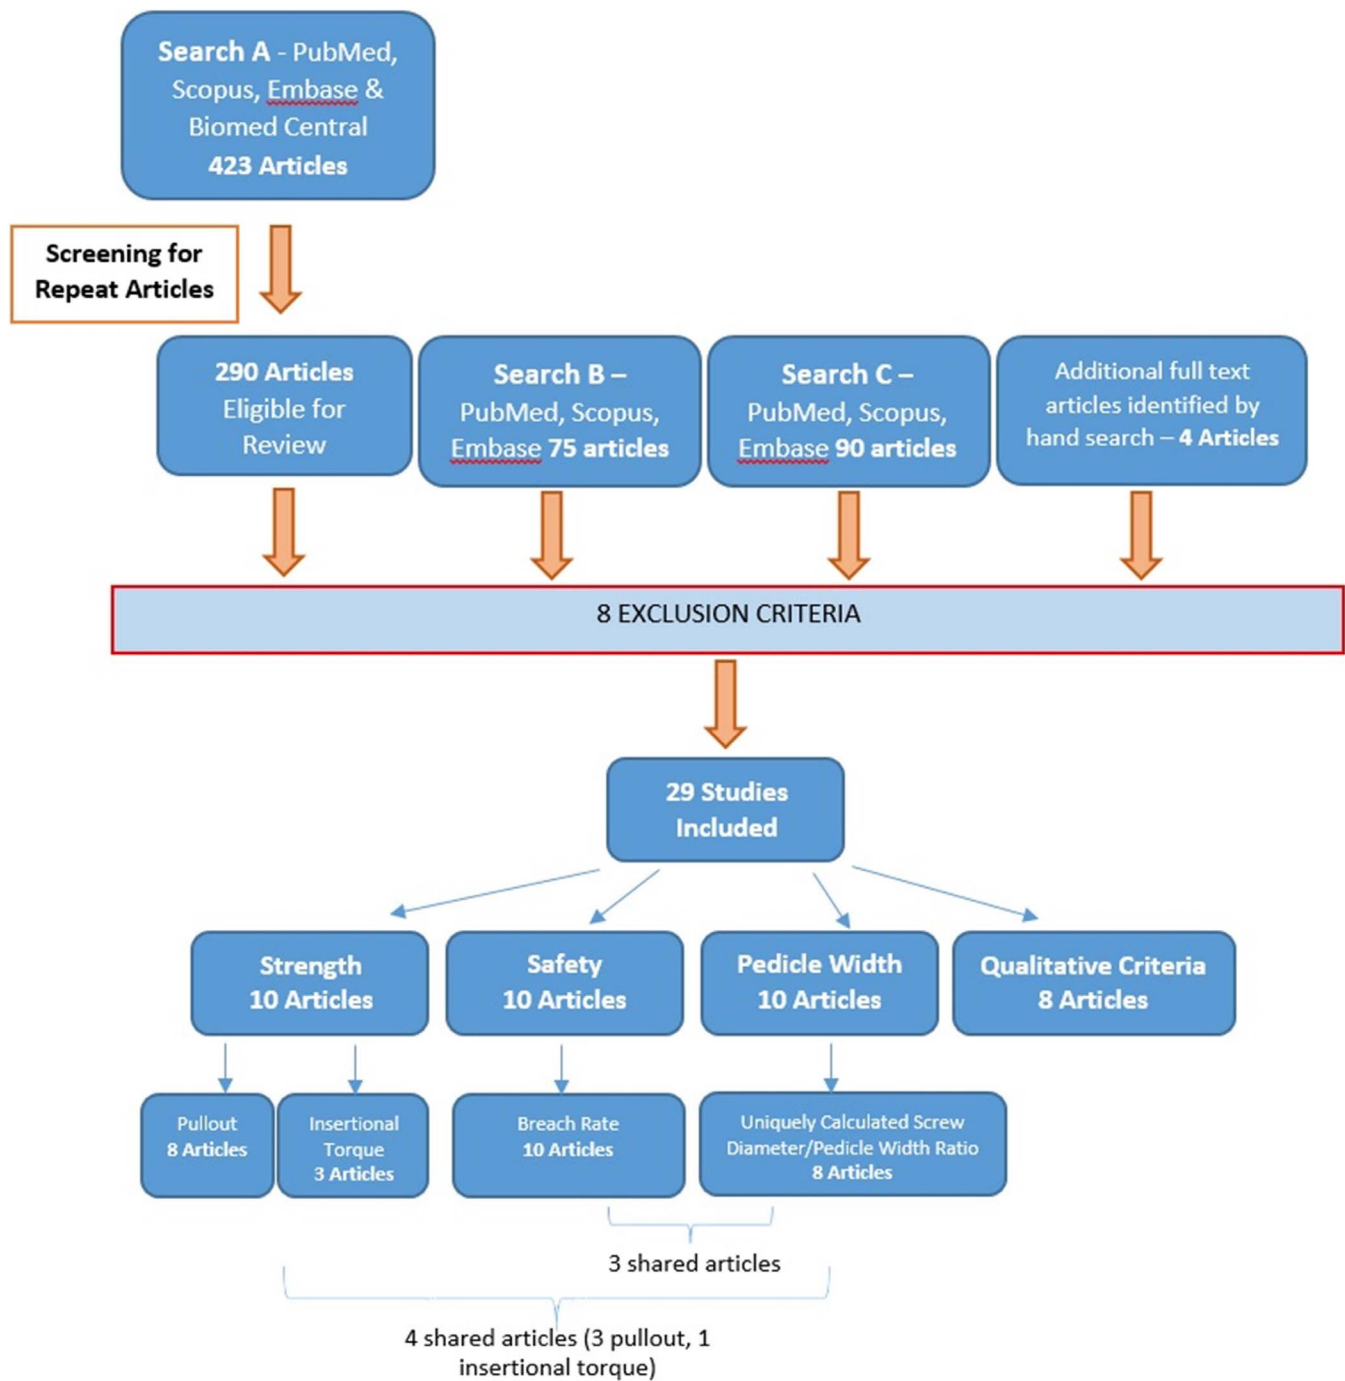


Figure 2. Systematic review procedure: the exclusion criteria allowed the narrowing to a limited number of papers with detailed information on pedicle width, breach rate, and fixation strength.

Of the 10 studies that concurrently reported PW and SD (Table 2), 5 also included measures of fixation strength, and 4 also include measures of breach rate. In an experimental study aimed at identifying criteria for safe diameter selection, Fujimoto et al,³² without specifying the insertion technique adopted, utilized SDs ranging from 4.0

to 6.5 mm and suggested that SDs should be 0.5 mm smaller than the PW. Helgeson et al²⁵ defined the optimal screw size as the screw size equal to, or the first size smaller than, the PW but did not achieve this size in all the tested specimens that were instrumented with the straightforward technique.

Table 1. Studies which offered recommendations for screw diameter (SD) in relation to pedicle width (PW): recommendations are reported with their relevant demographic to facilitate comparison across studies.

| Study | Recommendation | Insertion Technique | Subjects | Average Age | Range |
|-----------------------------------|--|---------------------|---------------------------------------|-------------|--------|
| Di Silvestre et al ²³ | SD should be 80% of PW. | Anatomical | Scoliosis patients | 33.4 | 12–54 |
| Suk et al ³⁷ | Ideal SD in adults is 80% of PW, but in children screws can be up to 115% of the PW. | Anatomical | Patients treated for spinal deformity | 18.5 | 2.7–70 |
| Takeshita et al ²⁴ | SD should not exceed 125% of PW. | Straightforward | Japanese scoliosis patients | 17.4 | 10–19 |
| Gstoettner et al ³⁶ | SD should not exceed 115% of PW. | Anatomical† | Scoliosis patients | | 9–28 |
| Lehman et al ³³ | SD chosen to achieve “70% pedicle fill.” | Not available | Generic cadaveric study | | 62–93 |
| Christodoulou et al ³⁵ | SD should closely match the internal trabecular PW and never exceed the external cortical PW. | Not available | Generic cadaveric study | 67.2 | 59–84 |
| Liau et al ³⁴ | SD should allow a 0.5 mm cortical margin on both the medial and lateral side to avoid fracture. | Anatomical† | Malaysian patients | | 18–80 |
| Kretzer et al ¹⁶ | SD should allow a 0.5 mm cortical margin on both the medial and lateral side to avoid fracture. | Straightforward‡ | Random US patients | | >18 |
| Fujimoto et al ³² | The size of the SD should be less than 0.5 mm smaller than the outer PW to be safely inserted in the pedicle cortex. | Not available | Japanese patients | 56 | 31–79 |

†Measure taken considering the pedicle axis as reference.

‡Measures taken to best approximate the straightforward.

Fixation Strength

Eight studies reported POS in relation to SD,^{10,22,25–27,38} 3 studies reported maximum insertional torque, and 1 study by Carmouche et al²¹ offered both measures (Table 3). Due to the heterogeneity of the patient populations (age, bone mineral density [BMD], living versus cadaveric, etc), screw insertion techniques, and testing methods, it is not possible to concurrently analyze results across studies. Screw diameters and POSs were often reported as an average across multiple levels, in some cases across the entire thoracic spine, making meaningful comparisons between vertebral level and/or screw sizes impractical across studies. In 4 pullout studies, however, we see a clear intrastudy relationship between increased SD and increased POS.^{21,22,25,39} A similar relationship is observed in the 3 studies of maximal insertional torque wherein Carmouche et al²¹ and Mishiro et al⁴⁰ report increases of 0.43 and 0.033 Nm of torque, respectively, with increasing SDs. The values reported by Matsukawa et al²⁸ appear to break this trend, but this can be accounted for by their use of a novel insertion trajectory that achieved greater cortical bone purchase with a smaller 5.5 mm screw as opposed to a 6.5 mm screw inserted in the standard straightforward technique. The influence of insertion technique on POS has been revealed by studies instrumenting the lower thoracic segments with SDs of about 5.5 mm that have shown higher pullout loads when inserted in the straightforward technique^{25,38} than in the anatomical trajectory.²⁷

Breach Ratio

Of the studies that reported breach rates in relation to SD, screw sizes ranged from 3.5 to 7.9 mm, and breach rates ranged from 100% at T3 with a 4.0 mm screw, to 0% at multiple levels with varying SDs (Table 4). Breach was defined differently by multiple studies. In Koktekir et al,⁴¹ greater than 25% of the outer SD needed to reside outside the pedicle wall in order to count as breach, whereas Fujimoto et al³² stated that a screw was either contained fully within the pedicle or was counted as breach. Most studies appear to follow the latter model of recording any perforation of the pedicle wall, and Payer et al⁵ states that, in their analysis, cases of questionable cortical integrity were counted as breach. Furthermore, Belmont et al⁴² states that medial perforations are safe up to 2 mm, while lateral perforations are safe up to 6 mm. Similarly, Chan et al²⁹ defines safe perforations as less than 2 mm. In the 5 studies that defined the safety of their breaches, only 10 of the 310 cumulative perforations, just 3.23%, were deemed unsafe.

Holly et al³⁰ reported breaches mainly in the segments T4–8, where screws 4 mm in diameter were placed in PWs ranging from 4.1 to 4.4 mm. Hart et al³¹ detailed PW values as well as breach rates. He used 4.0 and 4.5 mm screws and found lateral breach of 100% for 2.99 mm pedicles, which is reduced to 61% for PWs of 4.0 to 4.99 mm, and a minimal breach rate of 13% for PWs of 9.0 to 9.99 mm. Lastly, Fujimoto et al³² divided their specimens into 2 groups which warranted separate reporting in the table. Group 1 screws had a diameter less than the inner PW (ie, the transverse diameter of the

Table 2. Summary of data from studies concurrently reporting screw diameter and pedicle width.

| Study | Screw Diameter, mm (Vertebral Level) | Pedicle Width, mm (Vertebral Level) | Insertion Technique | Screw Length (mm) | Screw Type/Brand | Average Age (Range) | Sample Size |
|--|--|---|--------------------------|------------------------------|--|---------------------------|----------------|
| Chan et al ^{29a} | 5.0 (T1–6) 6.0 (T7–12) | 5.2 (T1) 4.9 (T2) 4.3 (T3) 4.2 (T4) 4.1 (T5) 4.4 (T6) 5.0 (T7) 4.9 (T8) 5.3 (T9) 6.3 (T10) 6.9 (T11) 6.6 (T12) | NA | NA | NA | NA | 240 |
| Holly et al ^{30a} | 4.0, 4.5, 5.5 (T1–12) | 4.4, 5.4, 7.9 (T1–12) | Anatomical ^c | NA | NA | NA | 64 |
| Helgeson et al ^{25b} | 5.0 ± 0.80 and 5.70 ± 1.05 (T1–12) | 6.96 ± 1.89 (T1–12) | Straightforward | NA | Monoaxial, Medtronic, Sofamor-Danek, Memphis, Tenn | NA | 15 |
| Liljenqvist et al ^{22b} | 4.8 and 5.5 (T4–8) 5.5, 6.5, and 7.2 (T9–12) | 5.1 ± 1.1 (T4) 5.0 ± 1.5 (T5) 5.1 ± 1.2 (T6) 5.4 ± 1.4 (T7) 6.0 ± 1.3 (T8) 6.6 ± 1.4 (T9) 7.4 ± 1.3 (T10) 8.8 ± 1.0 (T11) 8.7 ± 1.3 (T12) | NA | T4–8: 35–40; T9–12: 45–50 | Munster System, Schorndorf, Germany | 74.3 (60–89) | 45 |
| Hart et al ^{31a} | 4.0 (T1, T2) 4.0 (T4–7) 4.5 (T9, T10) | 8.4 ± 1.7 (T1, T2) 5.7 ± 1.6 (T4–7) 7.1 ± 1.5 (T9, T10) | Unique starting point | 30 | NA | NA | 129 |
| Fujimoto et al ^{32a} Group 1 | 4.7 ± 0.8 (T2) 4.0 ± 0.0 (T3) 5.5 ± 0.0 (T8) 5.5 ± 0.8 (T9) | 6.7 ± 0.3 (T2) 6.3 ± 0.2 (T3) 6.4 ± 0.2 (T8) 6.5 ± 0.4 (T9) | NA | NA | Vertex System, CD Horizon Legacy Spinal System, Medtronic Sofamor-Danek, Memphis, Tenn | 56 (31–79) | 16 |
| Group 2 | 4.2 ± 0.3 (T2) 4.0 ± 0.0 (T3) 4.5 ± 0.0 (T4) 4.2 ± 0.3 (T5) 4.7 ± 0.9 (T6) 5.5 ± 0.0 (T7) 5.3 ± 0.4 (T8) 4.5 ± 0.9 (T9) | 5.4 ± 0.4 (T2) 4.7 ± 0.4 (T3) 4.6 ± 0.4 (T4) 4.8 ± 0.9 (T5) 5.2 ± 1.1 (T6) 6.3 ± 0.2 (T7) 5.6 ± 0.2 (T8) 4.6 ± 1.2 (T9) | NA | NA | Vertex System, CD Horizon Legacy Spinal System, Medtronic Sofamor-Danek, Memphis, Tenn | 56 (31–79) | 22 |
| Xie et al ⁴⁶ | 5.5 (T1) 5.5 (T2) 5.0 and 5.5 (T3) 4.5, 5.0, and 5.5 (T4–6) 5.0 and 5.5 (T7, T8) | 5.0 ± 0.2 (T1) 4.7 ± 0.2 (T2) 4.3 ± 0.2 (T3) 3.3 ± 0.3 (T4) 3.3 ± 0.2 (T5) 3.1 ± 0.2 (T6) 3.7 ± 0.1 (T7) 3.9 ± 0.2 (T8) | Anatomical | 30–40 | NA | 9.2 (6–12) | 206 |
| Heller et al ^{26b} | 3.5 (T1–4) | 8.0 (T1) 7.0 (T2) 6.4 (T3) 6.4 (T4) | NA | NA | Cortical Screw, Synthes, West Chester, Pa | 75 (NA) | 35 |
| Hongo et al ^{27b} | 5.5 (T5–12) | 6.4 ± 1.6 (T5–12) | Anatomical | NA | Polyaxial, Abbott Spine, Bordeaux, France | 75.8 (±12) | 8 |
| Matsukawa et al ^{1b} | 5.5 or 6.5 (T9–12) | 6.0 ± 1.1 (T9) 6.8 ± 1.4 (T10) 8.6 ± 1.3 (T11) 9.1 ± 1.6 (T12) | Anatomical | 35–40 | Polyaxial SOLERA, Medtronic, Sofamor- Danek, Memphis, Tenn | 77.3 (65–83) | 44 |

Abbreviation: NA, not available.

^aFixation strength.^bBreach rate.^cNot disclosed but estimated from the figures shown.

Table 3. Summary of data from studies which reported screw diameter in relation to a measure of fixation strength.

| Study | Screw Diameter, mm (Vertebral Level) | Average Pullout Strength, N (Vertebral Level) | Max. Insertional Torque, Nm (Vertebral Level) | Insertion Technique | Screw Length, mm | Screw Type/Brand | Average Age (range) | Average BMD [g/cm ³] | Sample Size |
|---------------------------------|--|---|---|------------------------|-----------------------------------|--|---------------------------|--|----------------|
| Gayet et al ³⁹ | 4.0 or 5.0 (T1–12) | 820 ± 418, 1395 ± 435 (T1–12) | | NA | 40 | NA | 62 (NA) | Normal | 24 |
| Carmouche et al ⁵⁶ | 4.2 (T1–6) 5 (T7–12) | 288.2 (T1–6) 361.5 (T7–12) | | NA | NA | USS, Synthes West Chester, PA | NA | 0.833 | 102 |
| Helgeson et al ²⁵ | 5.0 (±0.80) or 5.70 (±1.05) (T1–12) | 712.3 ± 223.1, 877.9 ± 235.2 (T1–12) | | Straightforward | NA | Monoaxial, Medtronic Sofamor-Danek, Memphis, TN | NA | 0.6 ± 0.07 | 30 |
| Paik et al ³⁸ | 5 (T1–12) | Normal BMD = 1049 ± 202, osteoporotic = 813 ± 228 (T1–12) | | Straightforward | 35–45 | Polyaxial, CD Horizon Legacy Medtronic Sofamor-Danek | 81.5 (69–88) | 1.05, 0.563 | 15 |
| Heller et al ²⁶ | 3.5 (T1–4) | 775 (T1) 747.5 (T2) 596.0 (T3) 544.2 (T4) | | NA | NA | Cortical Screw, Synthes, West Chester, PA | 75 (NA) | NA | 35 |
| Liljenqvist et al ²² | 4.8 or 5.5 (T4–8) 5.5, 6.5 or 7.2 (T9–12) | 531.7 ± 213.8 (T4–8) 807.9 ± 207 (T9–12) | | NA | T4–8: 35–40 T9–12: 45–50 | Munster System, Schorndorf, Germany | 74.3 (60–89) | 1.097 | 45 |
| Brasiliense et al ¹⁰ | 4.5 (T6–11) | 839.6 ± 337.2 (T6–11) | | Straightforward | 50 | Pangea System, Medtronic Spinal and Biologics | 53 (32–82) | 0.674 | 10 |
| Hongo et al ²⁷ | 5.5 (T5–12) | 672 ± 412 (T5–12) | | Anatomical | NA | Polyaxial, Abbott Spine, Bordeaux France | 75.8 ± 12 | 0.8 ± 0.28 | 8 |
| Carmouche et al ⁵⁶ | 4.2 (T1–6) 5 (T7–12) | 1.36 (T1–6) 1.79 (T7–12) | | NA | 40 | USS, Synthes, West Chester, PA | NA | 0.833 | 102 |
| Mishiro et al ⁴⁰ | 3.5 and 4.0 (T1–12) | 0.550 (±0.116), 0.588 (T1–12) | | NA | NA | NA | 62.3 (48–70) | NA | 33 |
| Matsukawa et al ²⁸ | 5.5 and 6.5 (T9–12) | 1.02 (±0.25) and 0.66 (±0.15) (T9–12) | | Anatomical | 35–40 | Polyaxial Medtronic Sofamor-Danek, Memphis, TN | 77.3 (65–83) | NA | 44 |

Abbreviation: BMD, bone mass density, NA, not available.

Table 4. Summary of data from studies which reported screw diameter in relation to breach rate.

| Study | Screw Diameter, mm (Vertebral Level) | Breach Rate, % (Vertebral Level) | Insertion Technique | Screw Length (mm) | Average Age (Range) | Sample Size |
|--------------------------------|---|-------------------------------------|------------------------|-------------------------|---------------------------|----------------|
| Belmont et al ⁴² | 4.5 (T1) | 50 (T1) | NA | NA | 24 (6–56) | 279 |
| | 4.5 (T2) | 75 (T2) | | | | |
| | 4.5 (T3) | 60 (T3) | | | | |
| | 4.5 (T4) | 79 (T4) | | | | |
| | 4.5 (T5) | 79 (T5) | | | | |
| | 4.5 (T6) | 65 (T6) | | | | |
| | 4.5 (T7) | 55 (T7) | | | | |
| | 4.5 (T8) | 47 (T8) | | | | |
| | 4.5 (T9) | 43 (T9) | | | | |
| | 5.5 or 6.5 (T10) | 28 (T10) | | | | |
| | 5.5 or 6.5 (T11) | 25 (T11) | | | | |
| Koktekir et al ⁴¹ | 5.5 or 6.5 (T12) | 24 (T12) | NA | 30–50 | 56.5 (14–82) | 256 |
| | 4.0–5.0 (T1–12) | 0 (T1) | | | | |
| | | 0 (T1) | | | | |
| | | 0 (T2) | | | | |
| | | 0 (T3) | | | | |
| | | 0 (T4) | | | | |
| | | 0 (T5) | | | | |
| | | 0 (T6) | | | | |
| | | 0 (T7) | | | | |
| | | 0 (T8) | | | | |
| | | 0 (T9) | | | | |
| | | 2.40 (T10) | | | | |
| | | 4.20 (T11) | | | | |
| | | 1.50 (T12) | | | | |
| Cho et al ⁴⁵ | >7.7 (T1) | 100 (T1–12) | Anatomical | NA | 74.5 (61–82) | 162 |
| | >6.5 (T2) | | | | | |
| | >6.5 (T3) | | | | | |
| | >5.8 (T4) | | | | | |
| | >6.6 (T5) | | | | | |
| | >6.5 (T6) | | | | | |
| | >6.5 (T7) | | | | | |
| | >7.5 (T8) | | | | | |
| | >7.7 (T9) | | | | | |
| | >7.7 (T10) | | | | | |
| | >7.5 (T11) | | | | | |
| | >7.9 (T12) | | | | | |
| Holly et al ³⁰ | 4, 4.5 and 5.5 (T1–12) | 7.80 (T1–12) | †Anatomical | NA | NA | 64 |
| Chan et al ²⁹ | 5 (T1–6) | 10.40 (T1–12) | NA | NA | NA | 240 |
| Ranade et al ⁴³ | 6 (T7–12) | | NA | 25–30 | 4.6 (3.25–7.9) | 30 |
| | 3.5–5.5 (T1–12) | 0 (T1) | | | | |
| | | 25 (T2) | | | | |
| | | 0 (T3) | | | | |
| | | 0 (T4) | | | | |
| | | 0 (T5) | | | | |
| | | 0 (T6) | | | | |
| | | 0 (T10) | | | | |
| | | 25 (T11) | | | | |
| | | 12.50 (T12) | | | | |
| | | 16.70 (T1) | | | | |
| Mac-Thiong et al ⁴⁴ | 4.5 (T1–11) | 16.70 (T1) | Sagittal angle of 15° | 38 | NA “elderly” | 66 |
| | | 0 (T2) | | | | |
| | | 0 (T3) | | | | |
| | | 16.70 (T4) | | | | |
| | | 0 (T5) | | | | |
| | | 0 (T6) | | | | |
| | | 0 (T7) | | | | |
| | | 16.70 (T8) | | | | |
| | | 16.70 (T9) | | | | |
| | | 16.70 (T10) | | | | |
| | | 0 (T11) | | | | |
| Hart et al ³¹ | 4 (T1, T2) | 9 (T1, T2) | Unique starting point | 30 | NA | 129 |
| | 4 (T4–7) | 47 (T4–7) | | | | |
| | 4.5 (T9, T10) | 16 (T9, T10) | | | | |

Table 4. Continued.

| Study | Screw Diameter, mm (Vertebral Level) | Breach Rate, % (Vertebral Level) | Insertion Technique | Screw Length (mm) | Average Age (Range) | Sample Size |
|------------------------------|---|-------------------------------------|------------------------|-------------------------|---------------------------|----------------|
| Fujimoto et al ³² | | | | | | |
| Group 1 | 4.7 ± 0.8 (T2) | 0 (T1) | NA | NA | 56 (31–79) | 16 and 22 |
| | 4.0 ± 0.0 (T3) | 0 (T3) | | | | |
| | 5.5 ± 0.0 (T8) | 0 (T8) | | | | |
| Group 2 | 5.5 ± .8 (T9) | 14 (T9) | | | | |
| | 4.2 ± 0.3 (T2) | 33 (T2) | | | | |
| | 4.0 ± 0.0 (T3) | 100 (T3) | | | | |
| | 4.5 ± 0.0 (T4) | 67 (T4) | | | | |
| | 4.2 ± 0.3 (T5) | 50 (T5) | | | | |
| | 4.7 ± 0.9 (T6) | 75 (T6) | | | | |
| | 5.5 ± 0.0 (T7) | 0 (T7) | | | | |
| | 5.3 ± 0.4 (T8) | 50 (T8) | | | | |
| | 4.5 ± 0.9 (T9) | 67 (T9) | | | | |
| Payer et al ⁵ | 4.5 (T1–7) | 10 (T1–7) | Straightforward | 30–40 | 40 (20–65) | 62 |

Abbreviation: NA, not available.

inner cortical walls of the pedicle), while Group 2 screws had a diameter greater than the inner PW. According to the findings of Fujimoto et al,³² when SD is selected to be larger than the inner PW, the average breach rate can be as high as 54.5% but can be reduced to 6.3% for screws smaller than the inner PW.

Most of the studies reporting on breach rate did not provide any indication of the insertion technique adopted.^{43,44} However, a comparison can be made for a 4.5 mm SD inserted into the upper thoracic segments, for which the straightforward technique⁵ has shown higher breach rates than the anatomical trajectory.^{30,45}

Screw Diameter Selection in Relation to Pedicle Width

Of the 10 studies that concurrently reported PW and SD, Holly et al³⁰ and Liljenqvist et al²² were not included in SD/PW calculations because they reported nonspecific SDs across vertebral levels, making it impossible to calculate meaningful ratios by vertebral level. This left 8 studies with SD/PW ratios to report. In relation to PW, screws inserted with the straightforward technique²⁵ were smaller than screws adopted with the anatomical technique.^{27,46,47} Xie et al⁴⁶ provided their own SD/PW ratios with calculated standard deviations, so these were reported without additional calculation and can be considered exact.

Regardless of the insertion technique adopted, when we calculated the average SD/PW for each vertebral level, we found the lowest value at T1 with a ratio of 0.76 ± 0.29 (see Figure 3), which increased

through the midthoracic vertebrae to a peak of 1.02 ± 0.23 at T8 before decreasing towards T12 with a ratio of 0.83 ± 0.09 (Table 5).

The breach rate has been evaluated as being inversely proportional to the PW, with a coefficient of determination of 0.7 (see Figure 4). The smallest value of breach rate is associated with pedicles of 7.1 mm in width. Considering the entire thoracic spine, a weak correlation ($R^2 = 0.20$) has been found between the breach rate and the SD/PW ratio; however, the smallest values of breach rate are associated with the lower vertebrae T10–12, where very similar ratios within the range of 0.83 ± 0.05 to 0.84 ± 0.13 are used.

DISCUSSION

The data collected in this review allowed for an overview of SD selection in relation to vertebral level and insertion technique adopted. Despite our best efforts, there are some limitations of this review that should be mentioned. Gender of cadaveric and human subjects was rarely reported in the included studies, even though pedicle diameter has been clearly demonstrated to differ between men and women. As such, we were unable to consider the effect of this variation in our study. Additionally, screw design is clearly an important variable, especially for measures of fixation strength. Screw design and manufacturer were reported where available; however, many studies did not report on screw type. The variability of results among studies is almost certainly due in part to differences in screw design such as thread crest and pitch, which were

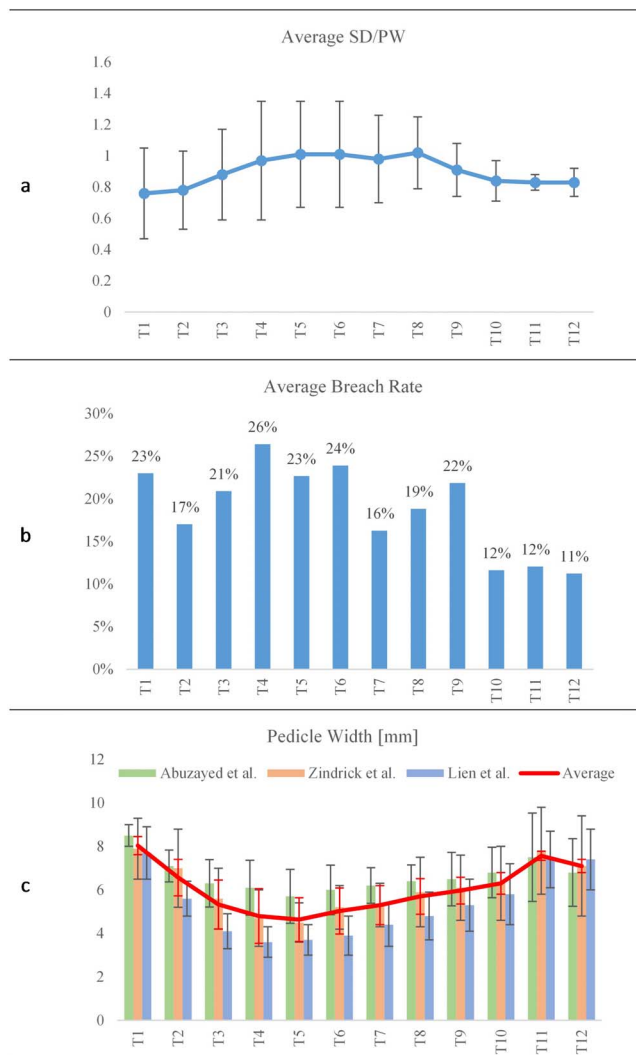


Figure 3. Average values calculated for screw diameter (SD) to pedicle width (PW), breach rate, and PW.

rarely reported, much less discussed by the included studies.

Furthermore, the SD in relation to PW is meaningless when insertion technique is not disclosed. For example, Helgeson et al,²⁵ using the straightforward technique, reports a mean POS of 877.9 ± 235.2 N with a calculated SD/PW of 0.82, while Hongo et al,²⁷ using the anatomical technique, reports a mean POS of 672 ± 412 N with a calculated SD/PW of 0.86. In addition, Helgeson et al²⁵ reported an average BMD of 0.6 ± 0.07 g/cm², while Hongo et al²⁷ reported an average BMD of 0.8 ± 0.28 g/cm², with the commonly accepted cutoff for osteoporosis stated as density less than 0.9g/cm². In cases of osteoporosis, BMD has been shown to strongly correlate with POS,³⁸ and the

large difference in reported POS between Gayet et al³⁹ and Carmouche et al²¹ with similar sized screws is likely due to the parallel difference in the BMD of their specimens. Studies such as Carmouche et al,²¹ cited in this review, have clearly demonstrated the correlation between increased insertional torque and increased pullout resistance in osteoporotic bone. This is likely due to the advantage it provides in achieving greater bony purchase of cortical bone, which can be highly variable between patients due to age,⁴⁸ as well as demonstrated differences between men and women.³⁴ In recent biomechanical studies, it has been demonstrated that the density of the bone in contact with the screw threads is strongly correlated with POS.^{49,50} As a result, the variable of SD can be seen as a means of achieving increased cortical bone purchase.

Breach rate peaked among found studies from T4–6 (see Figure 3b), which can be predicted by many studies which characterize T3–7 as having the smallest pedicles, with T5 often reported as the smallest overall.^{29,35,51} To confirm these relationships, we combined data from 3 frequently cited morphological studies of PW (see Figure 3c), which showed a minimum of 4.63 mm at T5 and a maximum of 7.57 mm at T11.^{52–54} A direct comparison of average breach rate by vertebral level with the average morphologic values of PW shows a clear inverse relationship between PW and breach rate (see Figure 4a). Considering the entire thoracic spine, a weak correlation ($R^2 = 0.20$) has been found between the breach rate and the SD/PW ratio (see Figure 4b), as seen in previous studies.^{29,31,32} Despite the poor correlation, breach rates associated with an SD/PW ratio of around 0.8 are consistently among the lowest overall. A ratio of 0.8 then can be reasonably suggested as a conservative starting point for SD selection for the inexperienced surgeon. When we consider the average SD/PW ratios calculated by vertebral level, we see an increase in ratio from T1 to T4 through T8 and a decrease in the lower thoracic spine towards T12. This can be accounted for by the fact that most studies do not make SD selections by individual segment, but rather utilize 1 or 2 SDs over multiple segments, or sometimes over the entire thoracic spine.^{25,38,55,56} The bandwidth in breach rates seen in Figure 3a can be reduced by greater specificity of screw selection by vertebral level. It should be noted that screw sizes available from the major manufacturers are limited, typically in 0.5 mm increments.

Table 5. Screw diameter (SD) to pedicle width (PW) ratios calculated in the current study (□ indicates studies also reporting on fixation strength and ◇ indicates studies also reporting on breach rate).

| Study | Insertion Technique | SD/PW Ratio (Vertebral Level) |
|---------------------------------|-----------------------|---|
| ◇ Chan et al ²⁸ | NA | 0.96 (T1) 1.02 (T2) 1.16 (T3) 1.19 (T4) 1.22 (T5) 1.14 (T6) 1.20 (T7) 1.22 (T8) 1.13 (T9) 0.95 (T10) 0.87 (T11) 0.91 (T12) |
| □ Helgeson et al ²⁵ | Straightforward | 0.72 and 0.82 (T1–12) |
| ◇ Hart et al ³¹ | Unique starting point | 0.48 (T1, T2) 0.7 (T4–7) 0.63 (T9, T10) |
| ◇ Fujimoto et al ³² | NA | 0.7 (T2) 0.63 (T3) 0.86 (T8) 0.85 (T9) |
| Group 1 | | 0.78 (T2) 0.85 (T3) 0.98 (T4) 0.88 (T5) 0.9 (T6) 0.87 (T7) 0.95 (T8) 0.98 (T9) |
| Group 2 | | 1.101 ± 0.051 (T1) 1.166 ± 0.042 (T2) 1.278 ± 0.050 (T3) 1.586 ± 0.0112 (T4) 1.596 ± 0.089 (T5) 1.640 ± 0.068 (T6) 1.444 ± 0.069 (T7) 1.390 ± 0.066 (T8) |
| □ Heller et al ²⁶ | NA | 0.44 (T1) 0.5 (T2) 0.55 (T3) 0.55 (T4) |
| □ Hongo et al ²⁷ | Anatomical | 0.86 (T5–12) |
| □ Matsukawa et al ²⁸ | Anatomical | 1.08 (T9) 0.96 (T10) 0.76 (T11) 0.71 (T12) |

Abbreviation: NA, not available.

Two studies in the current review specifically noted the inadequacy of current pedicle screw systems for instrumenting the midthoracic levels, with Liau et al³⁴ commenting that current systems are not suitable for the majority of the Malay population, and Gstoettner et al³⁶ concluding that one-third of midthoracic pedicles of scoliosis patients cannot be instrumented safely.

A final point of discussion we would like to propose is the clear difference in acceptable SD/PW in pediatric versus adult populations. Of the

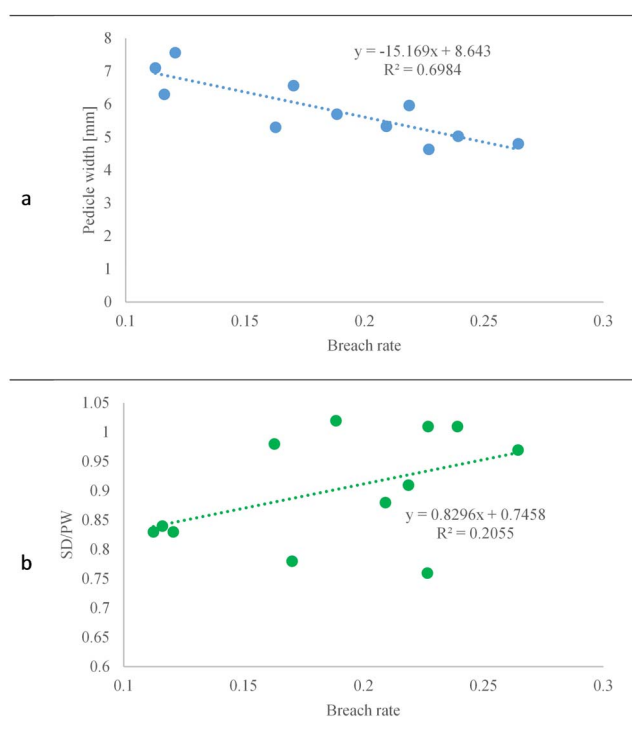


Figure 4. Breach rate correlation with (a) pedicle width and (b) screw diameter to pedicle width ratio.

qualitative studies found, 3 made SD/PW recommendations relevant for pediatric populations and averaged 1.18.^{24,36,37} These high SD/PW values can be explained by the relative plasticity of the pedicle cortex in the pediatric spine, which has been suggested to be capable of expanding 25% upon screw insertion.^{24,37}

CONCLUSIONS

A commonly accepted criteria for pedicle SD selection in adult thoracic fixation has yet to be proposed in the literature. Although 80% of the PW defines the SD as reported by several authors, this assertion is rarely reported for the midthoracic region of the spine. These vertebrae are characterized by relatively narrower pedicles where high pedicle breaches are usually found. This could be associated with the unavailability of SD sizes. In addition, fixation strength has been shown to be associated with BMD and cortical bone purchase, but it is not directly related to the SD/PW ratio. Based on this review of the literature, we believe that proper selection of the SD for individual vertebral level directly affects the insertion technique and the potential breach.

REFERENCES

1. Cuartas E, Rasouli A, O'Brien M, Shufflebarger HL. Use of all-pedicle-screw constructs in the treatment of adolescent idiopathic scoliosis. *J Am Acad Orthop Surg*. 2009;17(9):550–561.
2. Lykissas MG, Jain VV, Nathan ST, et al. Mid- to long-term outcomes in adolescent idiopathic scoliosis after instrumented posterior spinal fusion: a meta-analysis. *Spine (Phila Pa 1976)*. 2013;38(2):E113–E119. <https://doi.org/10.1097/BRS.0b013e31827ae3d0>.
3. Crawford AH, Lykissas MG, Gao X, Eismann E, Anadio J. All-pedicle screw versus hybrid instrumentation in adolescent idiopathic scoliosis surgery: a comparative radiographical study with a minimum 2-year follow-up. *Spine (Phila Pa 1976)*. 2013;38(14):1199–1208. <https://doi.org/10.1097/BRS.0b013e31828ce597>.
4. Hartl R, Theodore N, Dickman CA, Sonntag VKH. Technique of thoracic pedicle screw fixation for trauma. *Oper Tech Neurosurg*. 2004;7(1):22–30. <https://doi.org/10.1053/j.otsn.2004.04.005>.
5. Payer M. Unstable upper and middle thoracic fractures. Preliminary experience with a posterior transpedicular correction-fixation technique. *J Clin Neurosci*. 2005;12(5):529–533. <https://doi.org/10.1016/j.jocn.2004.11.006>.
6. Vanek P, Bradac O, Konopkova R, de Lacy P, Lacman J, Benes V. Treatment of thoracolumbar trauma by short-segment percutaneous transpedicular screw instrumentation: prospective comparative study with a minimum 2-year follow-up. *J Neurosurg Spine*. 2014;20(2):150–156. <https://doi.org/10.3171/2013.11.SPINE13479>.
7. Toyone T, Ozawa T, Inada K, et al. Short-segment fixation without fusion for thoracolumbar burst fractures with neurological deficit can preserve thoracolumbar motion without resulting in post-traumatic disc degeneration: a 10-year follow-up study. *Spine (Phila Pa 1976)*. 2013;38(17):1482–1490. <https://doi.org/10.1097/BRS.0b013e318297bdb7>.
8. Ebraheim NA, Georges J, Rongming X, Yeasting R. Anatomic relations of the thoracic pedicle to the adjacent neural structures. *Spine (Phila Pa 1976)*. 1997;22(14):1553–1556.
9. Sarwahi V, Suggs W, Wollowick AL, et al. Pedicle screws adjacent to the great vessels or viscera: a study of 2132 pedicle screws in pediatric spine deformity. *J Spinal Disord Tech*. 2014;27(2):64–69. <https://doi.org/10.1097/BSD.0b013e31825bfeec>.
10. Brasiliense LBC, Theodore N, Lazaro BCR, et al. Quantitative analysis of misplaced pedicle screws in the thoracic spine: how much pullout strength is lost? *J Neurosurg Spine*. 2010;12(5):503–508. <https://doi.org/10.3171/2009.11.SPINE09408>.
11. Hicks JM, Singla A, Shen FH, Arlet V. Complications of pedicle screw fixation in scoliosis surgery: a systematic review. *Spine (Phila Pa 1976)*. 2010;35(11):E465–E470. <https://doi.org/10.1097/BRS.0b013e3181d1021a>.
12. Gelalis ID, Paschos NK, Pakos EE, et al. Accuracy of pedicle screw placement: a systematic review of prospective in vivo studies comparing free hand, fluoroscopy guidance and navigation techniques. *Eur Spine J*. 2012;21(2):247–255. <https://doi.org/10.1007/s00586-011-2011-3>.
13. Kosmopoulos V, Schizas C. Pedicle screw placement accuracy: a meta-analysis. *Spine (Phila Pa 1976)*. 2007;32(3):E111–E120. <https://doi.org/10.1097/01.brs.0000254048.79024.8b>.
14. Wood M, Jason M. The surgical learning curve and accuracy of minimally invasive lumbar pedicle screw placement using CT based computer-assisted navigation plus continuous electromyography monitoring—a retrospective review of 627 screws in 150 patients. *Int J Spine Surg*. 2015;8:1–20.
15. Chen G, Li H, Li F, Chen W, Chen Q. Learning curve of thoracic pedicle screw placement using the free-hand technique in scoliosis: how many screws needed for an apprentice? *Eur Spine J*. 2012;21(6):1151–1156. <https://doi.org/10.1007/s00586-011-2065-2>.
16. Kretzer RM, Chaput C, Sciubba DM, et al. A computed tomography-based morphometric study of thoracic pedicle anatomy in a random United States trauma population. *J Neurosurg Spine*. 2011;14(2):235–243. <https://doi.org/10.3171/2010.9.SPINE1043>.
17. Fennell VS, Palejwala S, Skoch J, Stidd DA, Baaj AA. Freehand thoracic pedicle screw technique using a uniform entry point and sagittal trajectory for all levels: preliminary clinical experience. *J Neurosurg Spine*. 2014;21(5):778–784. <https://doi.org/10.3171/2014.7.SPINE1489>.
18. Kim YJ, Lenke LG, Bridwell KH, Cho YS, Riew KD. Free hand pedicle screw placement in the thoracic spine: is it safe? *Spine (Phila Pa 1976)*. 2004;29(3):333–342; discussion 342. <https://doi.org/10.1097/01.BRS.0000109983.12113.9B>.
19. Nottmeier EW, Seemer W, Young PM. Placement of thoracolumbar pedicle screws using three-dimensional image guidance: experience in a large patient cohort. *J Neurosurg Spine*. 2009;10(1):33–39. <https://doi.org/10.3171/2008.10.SPI08383>.
20. Rampersaud YR, Simon DA, Foley KT. Accuracy requirements for image-guided spinal pedicle screw placement. *Spine (Phila Pa 1976)*. 2001;26(4):352–359.
21. Carmouche JJ, Molinari RW, Gerlinger T, Devine J, Patience T. Effects of pilot hole preparation technique on pedicle screw fixation in different regions of the osteoporotic thoracic and lumbar spine. *J Neurosurg Spine*. 2005;3(5):364–370. <https://doi.org/10.3171/spi.2005.3.5.0364>.
22. Liljenqvist U, Hackenberg L, Link T, Halm H. Pullout strength of pedicle screws versus pedicle and laminar hooks. *Acta Orthop Belg*. 2001;67(2):3–9.
23. Di Silvestre M, Parisini P, Lolli F, Bakaloudis G. Complications of thoracic pedicle screws in scoliosis treatment. *Spine (Phila Pa 1976)*. 2007;32(15):1655–1661. <https://doi.org/10.1097/BRS.0b013e318074d604>.
24. Takeshita K, Maruyama T, Chikuda H, et al. Diameter, length, and direction of pedicle screws for scoliotic spine: analysis by multiplanar reconstruction of computed tomography. *Spine (Phila Pa 1976)*. 2009;34(8):798–803. <https://doi.org/10.1097/BRS.0b013e3181895c36>.
25. Helgeson MD, Kang DG, Lehman RA, Dmitriev AE, Luhmann SJ. Tapping insertional torque allows prediction for better pedicle screw fixation and optimal screw size selection. *Spine J*. 2013;13(8):957–965. <https://doi.org/10.1016/j.spinee.2013.03.012>.
26. Heller JG, Shuster JK, Hutton WC. Pedicle and transverse process screws of the upper thoracic spine: biomechanical comparison of loads to failure. *Spine (Phila Pa 1976)*. 1999;24(7):654–658.

27. Hongo M, Ilharreborde B, Gay RE, et al. Biomechanical evaluation of a new fixation device for the thoracic spine. *Eur Spine J*. 2009;18(8):1213–1219.
28. Matsukawa K, Yato Y, Hynes RA, et al. Cortical bone trajectory for thoracic pedicle screws: a technical note. *J Spinal Disord Tech*. 2014. <https://doi.org/10.1097/BSD.0000000000000130>.
29. Chan CYW, Kwan MK, Saw LB. Thoracic pedicle screw insertion in Asian cadaveric specimen: does radiological pedicle profile affect outcome? *Surg Radiol Anat*. 2011;33(1):19–25. <https://doi.org/10.1007/s00276-010-0726-1>.
30. Holly LT, Foley KT. Three-dimensional fluoroscopy-guided percutaneous thoracolumbar pedicle screw placement. *J Neurosurg Spine*. 2003;99(3 Suppl):324–329.
31. Hart RA, Hansen BL, Shea M, Hsu F, Anderson GJ. Pedicle screw placement in the thoracic spine: a comparison of image-guided and manual techniques in cadavers. *Spine (Phila Pa 1976)*. 2005;30(12):E326–E331.
32. Fujimoto T, Sei A, Taniwaki T, Okada T, Yakushiji T, Mizuta H. Pedicle screw diameter selection for safe insertion in the thoracic spine. *Eur J Orthop Surg Traumatol*. 2011;22(5):351–356. <https://doi.org/10.1007/s00590-011-0846-2>.
33. Lehman R a, Polly DW, Kuklo TR, Cunningham B, Kirk KL, Belmont PJ. Straight-forward versus anatomic trajectory technique of thoracic pedicle screw fixation: a biomechanical analysis. *Spine (Phila Pa 1976)*. 2003;28(18):2058–2065. <https://doi.org/10.1097/01.BRS.0000087743.57439.4F>.
34. Liao KM, Yusof MI, Abdullah MS, Abdullah S, Yusof AH. Computed tomographic morphometry of thoracic pedicles: safety margin of transpedicular screw fixation in Malaysian Malay population. *Spine (Phila Pa 1976)*. 2006;31(16):E545–E550.
35. Christodoulou AG, Apostolou T, Ploumis A, Terzidis I, Hantzokos I, Pournaras J. Pedicle dimensions of the thoracic and lumbar vertebrae in the Greek population. *Clin Anat*. 2005;18(6):404–408.
36. Gstoeitner M, Lechner R, Glodny B, Thaler M, Bach CM. Inter- and intraobserver reliability assessment of computed tomographic 3D measurement of pedicles in scoliosis and size matching with pedicle screws. *Eur Spine J*. 2011;20(10):1771–1779. <https://doi.org/10.1007/s00586-011-1908-1>.
37. Suk S-I, Kim W-J, Lee S-M, Kim J-H, Chung E-R. Thoracic pedicle screw fixation in spinal deformities. *Spine (Phila Pa 1976)*. 2001;26(18):2049–2057. <https://doi.org/10.1097/00007632-200109150-00022>.
38. Paik H, Kang DG, Lehman RA, Gaume RE, Ambati D V, Dmitriev AE. The biomechanical consequences of rod reduction on pedicle screws: should it be avoided? *Spine J*. 2013;13(11):1617–1626.
39. Gayet L, Pries P, Hamcha H, Clarac J-P, Texereau J. Biomechanical study and digital modeling of traction resistance in posterior thoracic implants. *Spine (Phila Pa 1976)*. 2002;27(7):707–714.
40. Mishiro T, Sairyo K, Shinohara A, Chikawa T, Kosaka H, Dezawa A. Assessment of maximal insertional torque of cervical and thoracic screws during posterior spinal surgery. *J Med Investig*. 2014;61(3–4):393–398.
41. Koktekir E, Ceylan D, Tatarli N, Karabagli H, Recber F, Akdemir G. Accuracy of fluoroscopically-assisted pedicle screw placement: analysis of 1,218 screws in 198 patients. *Spine J*. 2014;14(8):1702–1708. <https://doi.org/10.1016/j.spinee.2014.03.044>.
42. Belmont PJ, Kemme W, Dhavan A, Polly D. In vivo accuracy of thoracic pedicle screws. *Spine (Phila Pa 1976)*. 2001;26(21):2340–2346.
43. Ranade A, Samdani AF, Williams R, et al. Accuracy of pedicle screws in children younger than eight years of age. *Spine (Phila Pa 1976)*. 2009;34(26):2907–2911. <https://doi.org/10.1097/BRS.0b013e3181b77af3>.
44. Mac-Thiong J-M, Labelle H, Rooze M, Feipel V, Aubin C-E. Evaluation of a transpedicular drill guide for pedicle screw placement in the thoracic spine. *Eur Spine J*. 2003;12(5):542–547.
45. Cho SK, Skovrlj B, Lu Y, Caridi JM, Lenke LG. The effect of increasing pedicle screw size on thoracic spinal canal dimensions: an anatomic study. *Spine (Phila Pa 1976)*. 2014;39(20):E1195–E1200. <https://doi.org/10.1097/BRS.0000000000000514>.
46. Xie J, Wang Y, Zhao Z, Zhang Y. The safe placement of upper and middle thoracic pedicle screws in pediatric deformity. *J Spinal Disord Tech*. 2011;24(1):55–59. <https://doi.org/10.1097/BSD.0b013e3181d4c877>.
47. Matsukawa K, Yato Y, Kato T, Imabayashi H, Asazuma T, Nemoto K. In vivo analysis of insertional torque during pedicle screwing using cortical bone trajectory technique. *Spine (Phila Pa 1976)*. 2014;39(4):E240–E245. <https://doi.org/10.1097/BRS.0000000000000116>.
48. Zhuang Z, Xie Z, Ding S, et al. Evaluation of thoracic pedicle morphometry in a Chinese population using 3D reformatted CT. *Clin Anat*. 2012;25(4):461–467. <https://doi.org/10.1002/ca.21265>.
49. Amirouche F, Solitro GF, Magnan BP. Stability and spine pedicle screws fixation strength—a comparative study of bone density and insertion angle. *Spine Deform*. 2016;4(4):261–267. <https://doi.org/10.1016/j.jspsd.2015.12.008>.
50. Chou W-K, Chien A, Wang J-L. Pullout strength of thoracic pedicle screws improved with cortical bone ratio: a cadaveric study. *J Orthop Sci*. 2014;19(6):900–906. <https://doi.org/10.1007/s00776-014-0614-3>.
51. Kim J-H, Choi G-M, Chang I-B, Ahn S-K, Song J-H, Choi H-C. Pedicular and extrapedicular morphometric analysis in the Korean population: computed tomographic assessment relevance to pedicle and extrapedicle screw fixation in the thoracic spine. *J Korean Neurosurg Soc*. 2009;46(3):181–188.
52. Abuzayed B, Tutunculer B, Kucukyuruk B, Tuzgen S. Anatomic basis of anterior and posterior instrumentation of the spine: morphometric study. *Surg Radiol Anat*. 2010;32(1):75–85. <https://doi.org/10.1007/s00276-009-0545-4>.
53. Zindrick MR, Wiltse LL, Doornik A, et al. Analysis of the morphometric characteristics of the thoracic and lumbar pedicles. *Spine (Phila Pa 1976)*. 1987;12(2):160–166. <https://doi.org/10.1097/00007632-198703000-00012>.
54. Lien S-B, Liou N-H, Wu S-S. Analysis of anatomic morphometry of the pedicles and the safe zone for through-pedicle procedures in the thoracic and lumbar spine. *Eur Spine J*. 2007;16(8):1215–1222. <https://doi.org/10.1007/s00586-006-0245-2>.
55. Brasiense LBC, Theodore N, Lazaro BCR, et al. Quantitative analysis of misplaced pedicle screws in the thoracic

spine: how much pullout strength is lost? Presented at the 2009 Joint Spine Section Meeting. *J Neurosurg Spine*. 2010;12(5):503–508. <https://doi.org/10.3171/2009.11.SPINE09408>.

56. Carmouche JJ, Molinari RW, Gerlinger T, Devine J, Patience T. Effects of pilot hole preparation technique on pedicle screw fixation in different regions of the osteoporotic thoracic and lumbar spine. *J Neurosurg Spine*. 2005;3(5):364–370.

Corresponding Author: Ankit Mehta, MD,
Department of Neurosurgery, University of Illinois

at Chicago, 912 S Wood St, Chicago, IL 60612.
Phone: (312) 996-4842; Fax: (312) 996-6497; Email:
ankitm@uic.edu.

Published 0 Month 2019

This manuscript is generously published free of charge by ISASS, the International Society for the Advancement of Spine Surgery. Copyright © 2018 ISASS. To see more or order reprints or permissions, see <http://ijssurgery.com>.